

1/8


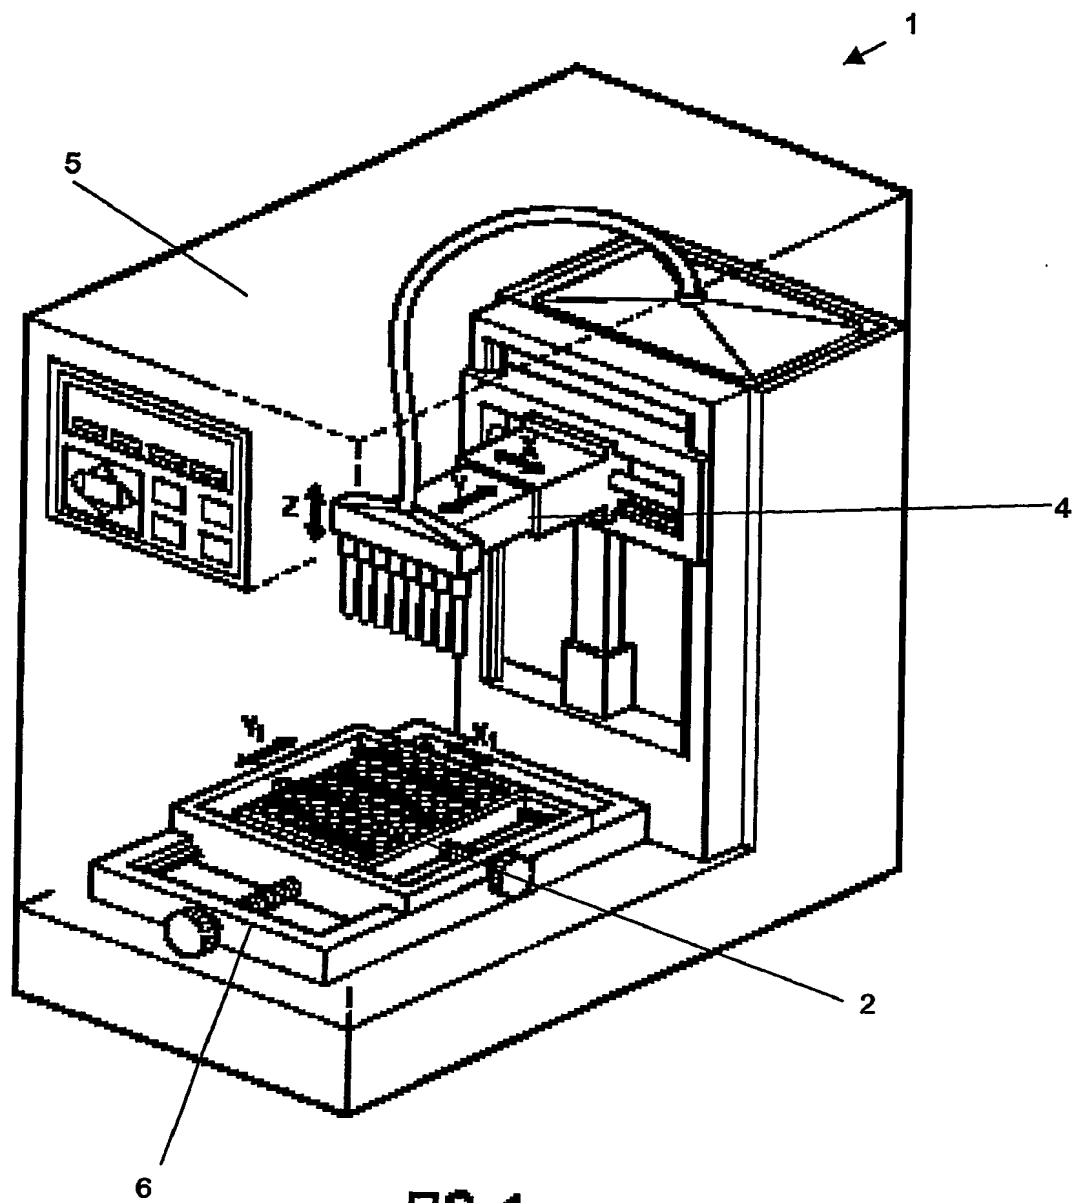


FIG. 1

2/8

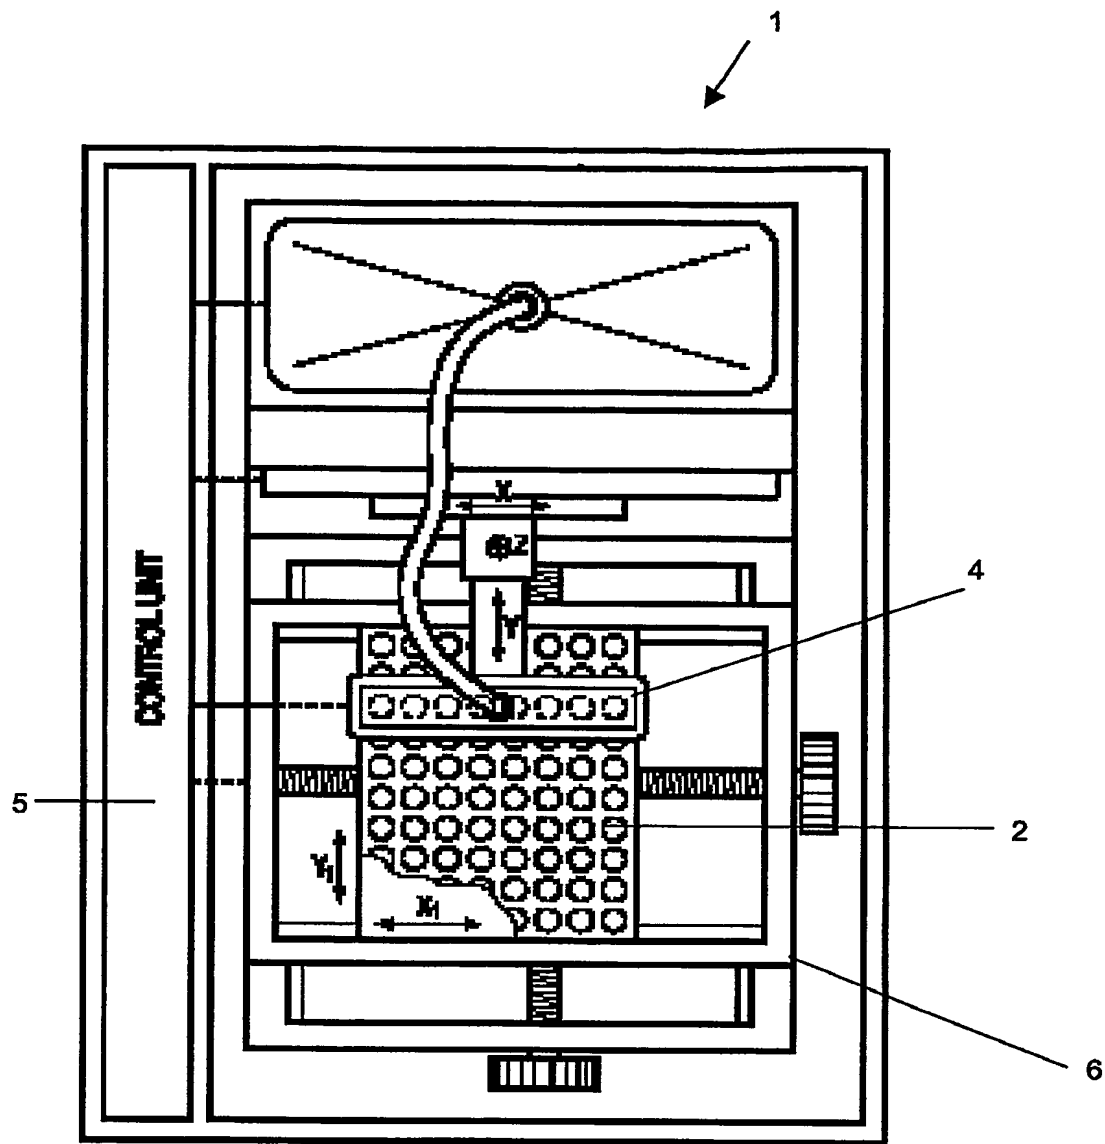

3/8

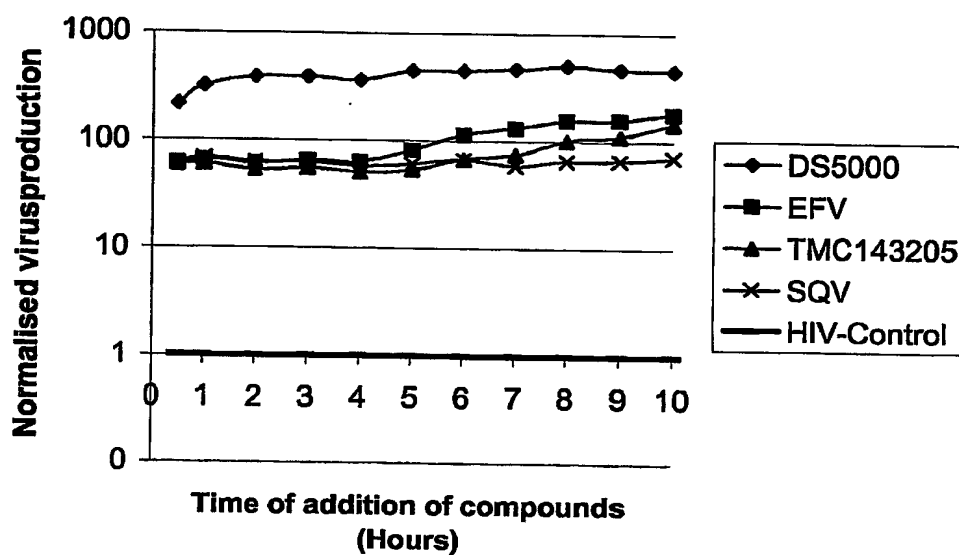


Figure 3

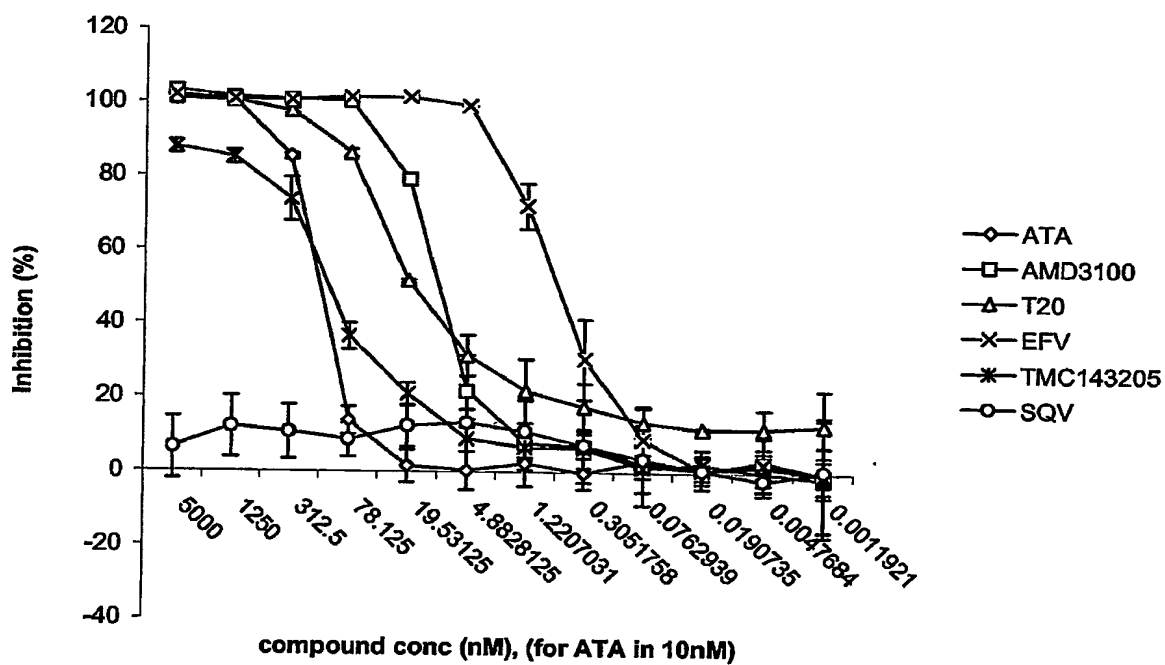


Figure 4

4/8

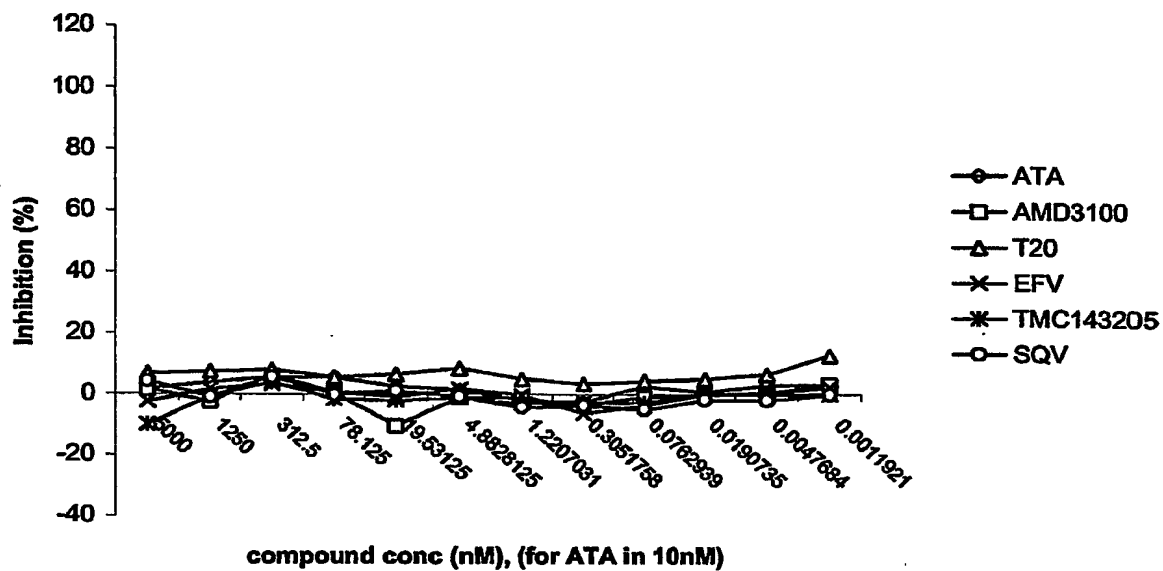


Figure 5

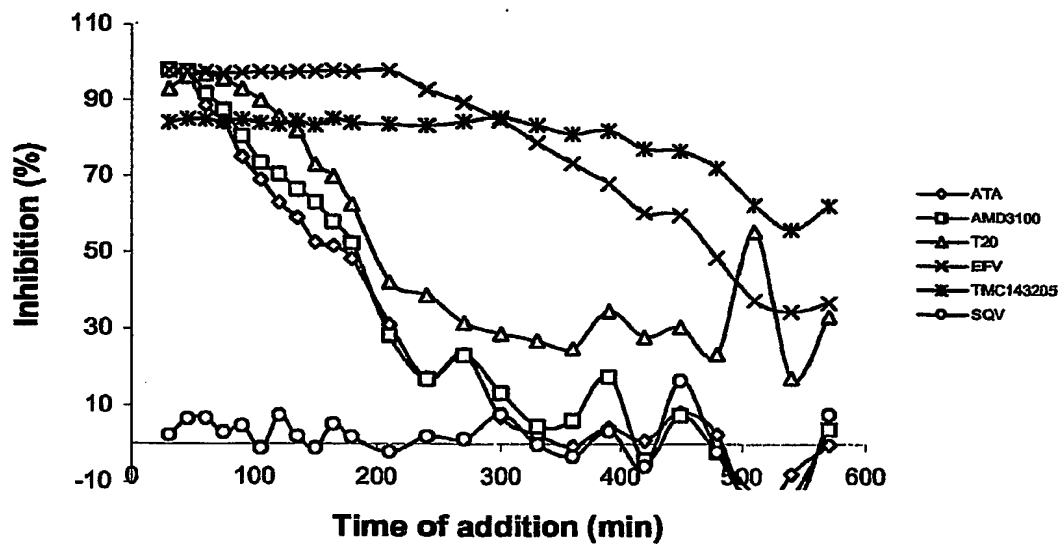


Figure 6

5/8


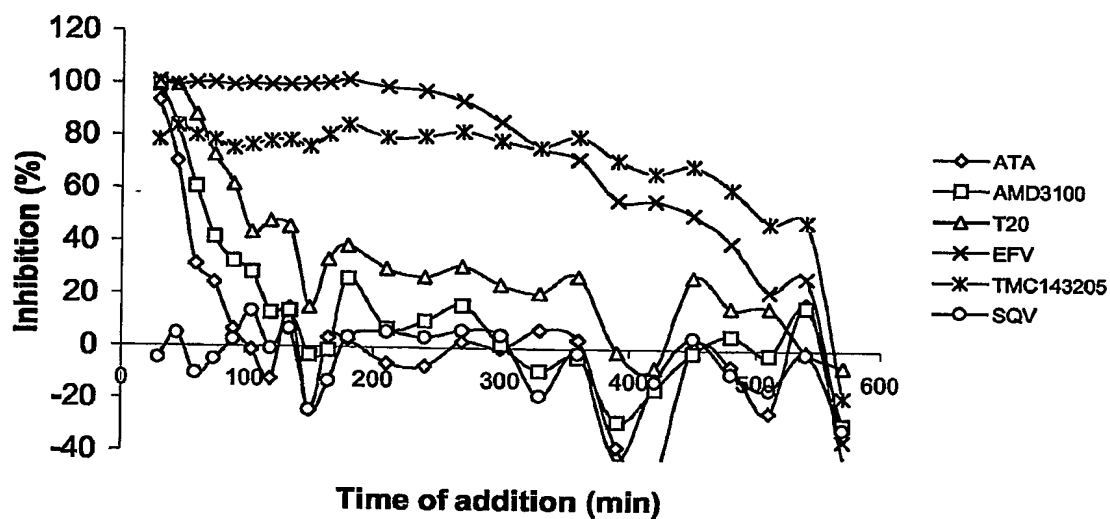


Figure 7

Time (min) 30 60 90 120 180 240 300 360 420 480 540 600

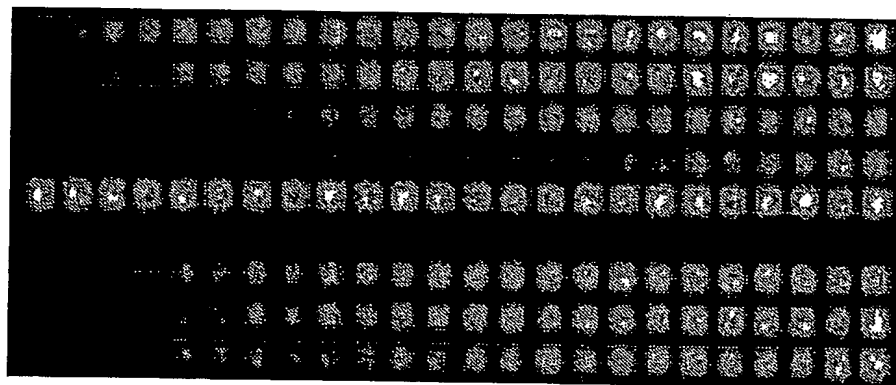

CD4-inhibitor  
X4-inhibitor  
Fusion-inhibitor  
RT  
Virus control  
Cell control  
Test-compounds

Figure 8

BEST AVAILABLE COPY

6/8

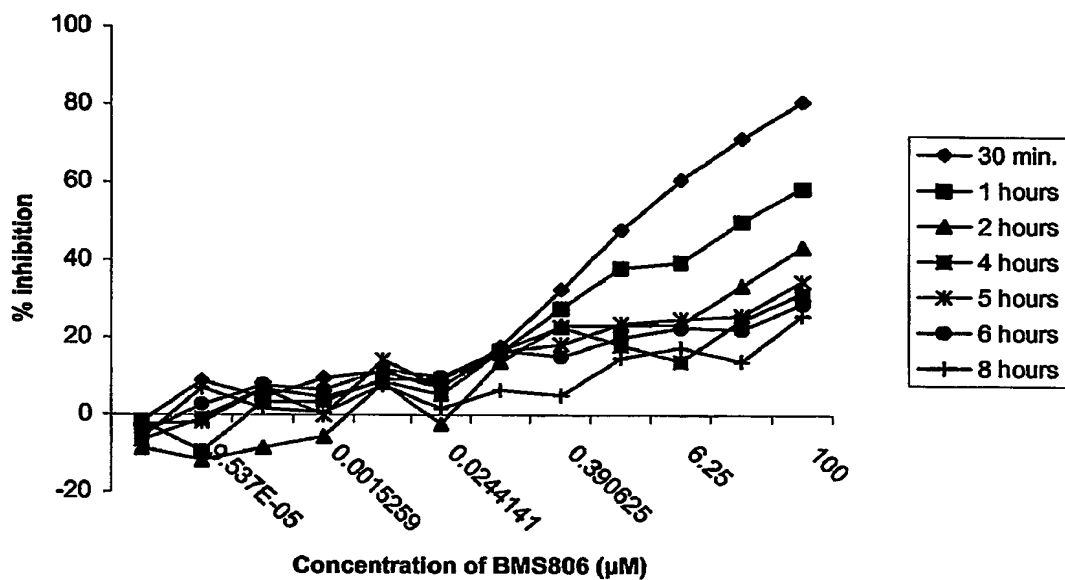
Anti-viral-experiment with TOA protocol: **23°C**

Figure 9A

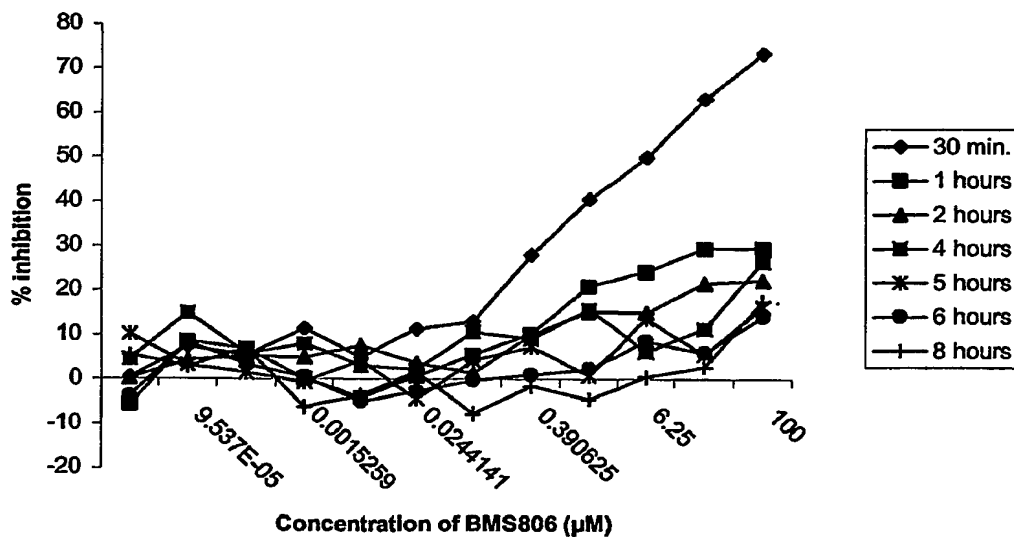
Anti-viral-experiment with TOA protocol: **37°C**

Figure 9B

7/8

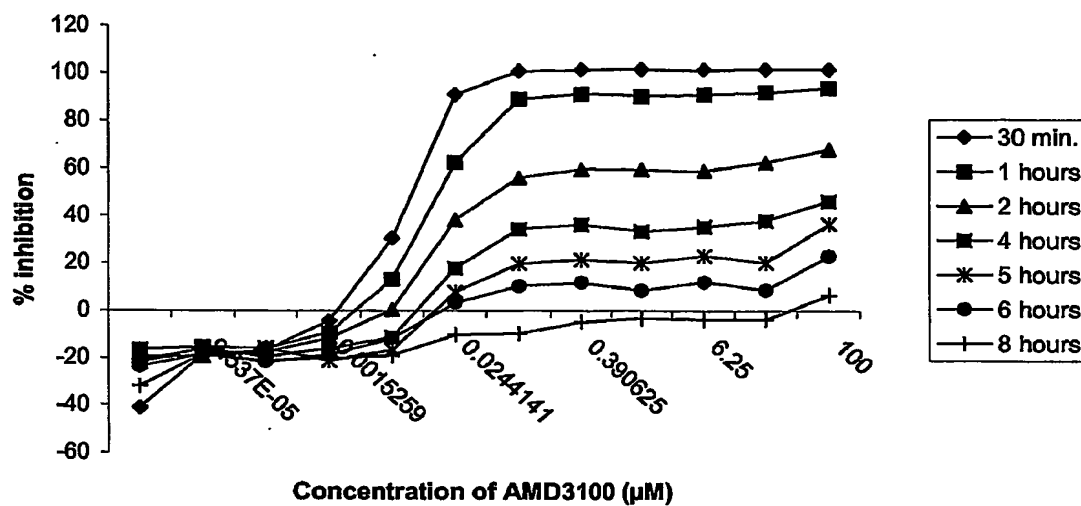
Anti-viral-experiment with TOA protocol: **23°C**

Figure 10A

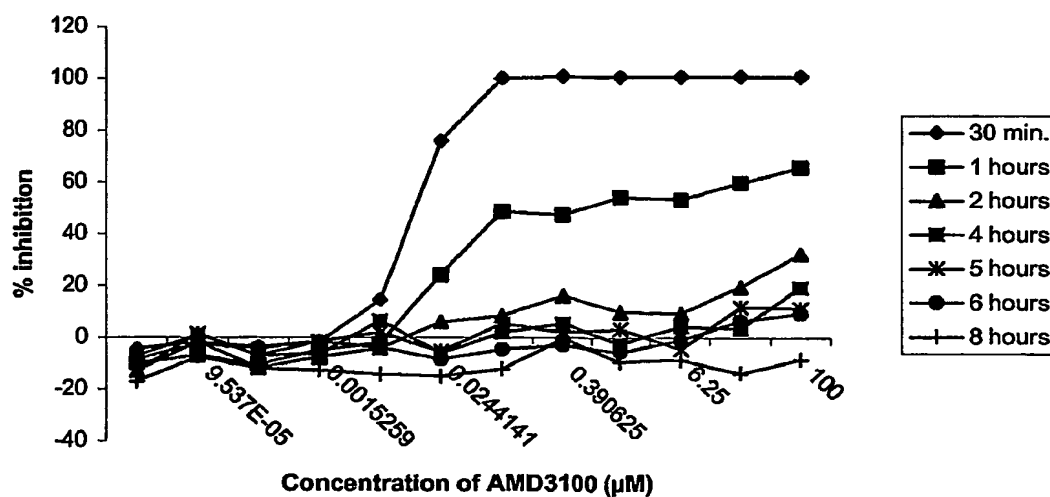
Anti-viral-experiment with TOA protocol: **37°C**

Figure 10B

8/8

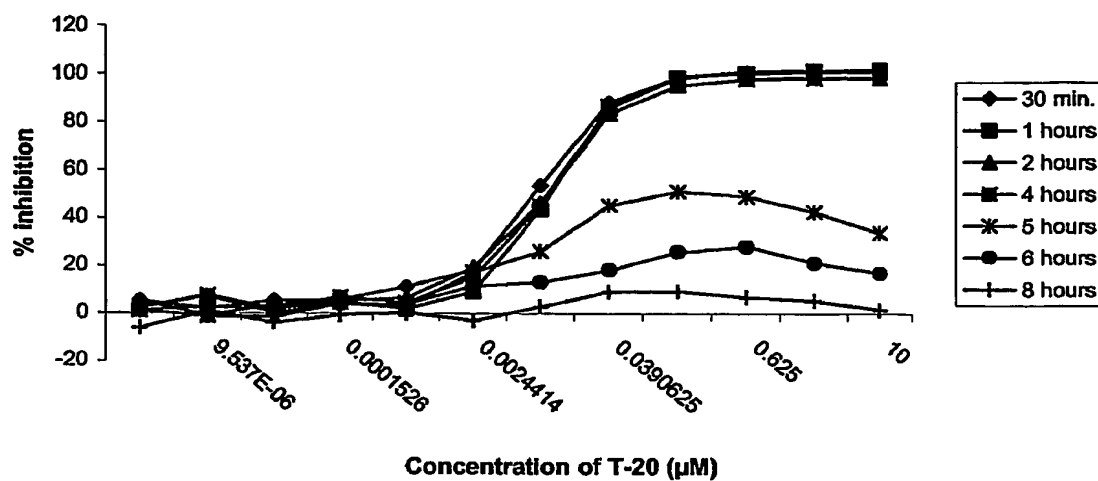
Anti-viral-experiment with TOA protocol: **23°C**

Figure 11A

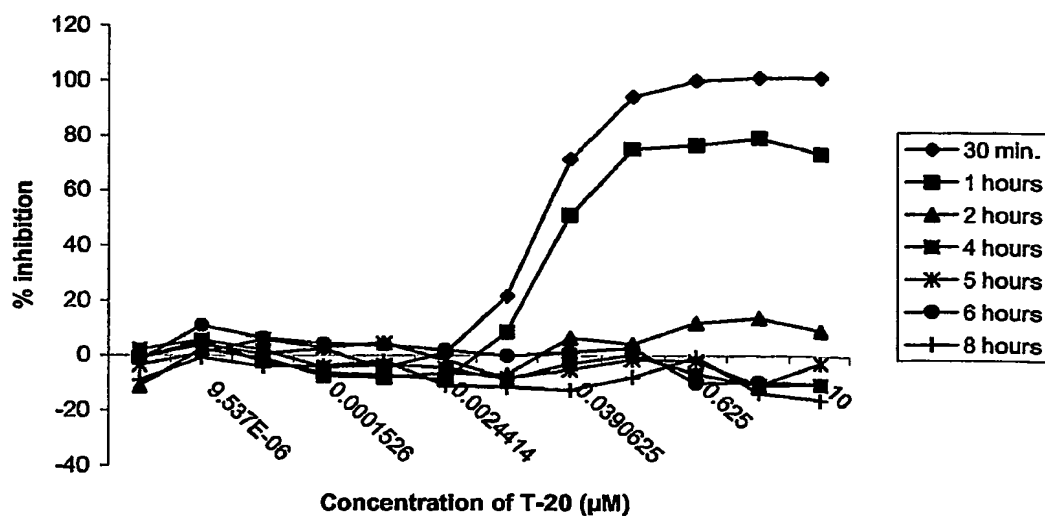
Anti-viral-experiment with TOA protocol: **37°C**

Figure 11B